



An evaluation tool kit of air quality micro-sensing units



Barak Fishbain ^{a,*}, Uri Lerner ^{a,1}, Nuria Castell ^b, Tom Cole-Hunter ^{c,d}, Olalekan Popoola ^e, David M. Broday ^a, Tania Martinez Iñiguez ^{c,d}, Mark Nieuwenhuijsen ^c, Milena Jovasevic-Stojanovic ^f, Dusan Topalovic ^{f,g}, Roderic L. Jones ^e, Karen S. Galea ^h, Yael Etzion ^a, Fadi Kizel ^a, Yaela N. Golumbic ^{a,i}, Ayelet Baram-Tsabari ⁱ, Tamar Yacobi ^a, Dana Drahler ^a, Johanna A. Robinson ^{j,m}, David Kocman ^j, Milena Horvat ^j, Vlasta Svecova ^k, Alexander Arpacı ^l, Alena Bartonova ^b

^a The Technion Center of Excellence in Exposure Science and Environmental Health (TCEEH), Faculty of Civil and Environmental Engineering, Technion – Israel Institute of Technology, Haifa, Israel

^b Norwegian Institute for Air Research (NILU), Kjeller, Norway

^c ISGlobal, Centre for Research in Environmental Epidemiology (CREAL), Barcelona, Spain

^d Centro de Investigación Biomédica en Red de Epidemiología y Salud Pública (CIBERESP), Madrid, Spain

^e Centre for Atmospheric Science, Department of Chemistry, University of Cambridge, Cambridge, England, UK

^f VINČA Institute of Nuclear Sciences, University of Belgrade, Belgrade, Serbia

^g School of Electrical Engineering, University of Belgrade, Belgrade, Serbia

^h Centre for Human Exposure Science, Institute of Occupational Medicine (IOM), Edinburgh, Scotland, UK

ⁱ Faculty of Education in Science and Technology, Technion – Israel Institute of Technology, Haifa, Israel

^j Department of Environmental Sciences, Jožef Stefan Institute, Ljubljana, Slovenia

^k Department of Genetic Ecotoxicology, Institute of Experimental Medicine AS CR, Prague, Czech Republic


^l UBIMET GmbH, Vienna, Austria

^m Jožef Stefan International Postgraduate School, Ljubljana, Slovenia

HIGHLIGHTS

- A comprehensive evaluation of modern approach to air-quality (AQ) monitoring
- AQ micro sensing units (MSUs) performance assessment in a range of applications
- Four new assessment measures that highlight new sensors' performance aspects
- Comprehensive assessment of AQ MSU network across Europe
- In-depth understating of MSU functionality via large scale comparative analysis

GRAPHICAL ABSTRACT

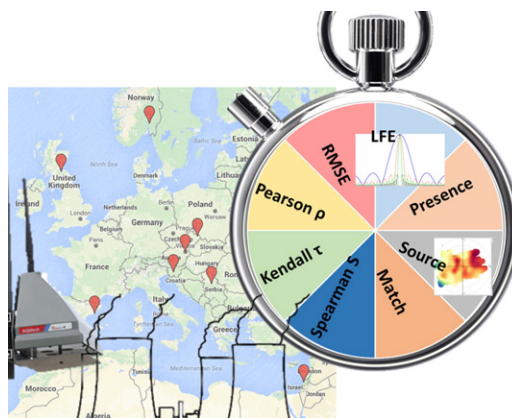

ARTICLE INFO

Article history:

Received 3 July 2016

Received in revised form 5 September 2016

ABSTRACT

Recent developments in sensory and communication technologies have made the development of portable air-quality (AQ) micro-sensing units (MSUs) feasible. These MSUs allow AQ measurements in many new applications, such as ambulatory exposure analyses and citizen science. Typically, the performance of these devices is

* Corresponding author.

E-mail address: fishbain@technion.ac.il (B. Fishbain).

¹ Equally contributed.

Accepted 8 September 2016
Available online 24 September 2016

Editor: J Jay Gan

Keywords:

Air quality
Environmental monitoring
Micro sensing units
Wireless distributed sensor network
Sensors performance

assessed using the mean error or correlation coefficients with respect to a laboratory equipment. However, these criteria do not represent how such sensors perform outside of laboratory conditions in large-scale field applications, and do not cover all aspects of possible differences in performance between the sensor-based and standardized equipment, or changes in performance over time. This paper presents a comprehensive Sensor Evaluation Toolbox (SET) for evaluating AQ MSUs by a range of criteria, to better assess their performance in varied applications and environments. Within the SET are included four new schemes for evaluating sensors' capability to: locate pollution sources; represent the pollution level on a coarse scale; capture the high temporal variability of the observed pollutant and their reliability. Each of the evaluation criteria allows for assessing sensors' performance in a different way, together constituting a holistic evaluation of the suitability and usability of the sensors in a wide range of applications. Application of the SET on measurements acquired by 25 MSUs deployed in eight cities across Europe showed that the suggested schemes facilitates a comprehensive cross platform analysis that can be used to determine and compare the sensors' performance. The SET was implemented in R and the code is available on the first author's website.

© 2016 Elsevier B.V. All rights reserved.

1. Introduction

Air pollution is recognized as a contributing factor to various health outcomes, and has been associated with public health risks (International Agency for Research on Cancer (IARC), 2013; Sarnat et al., 2000). Accurately assessing ambient concentrations of different air pollutants is necessary in any study on the impact of air quality (AQ) on different health endpoints. To date, ambient pollutant concentrations are obtained from either short time-period measurement campaigns using a large number of sensing devices (e.g. (Crouse et al., 2009)), or from measurements reported by standard Air Quality Monitoring (AQM) stations over extended time periods (e.g. (Pope et al., 2002)). While the former is limited in temporal representativeness (e.g. due to inter-seasonal variation), the latter is limited in spatial representativeness (e.g. due to dispersion patterns) and typically measures only a limited number of criteria pollutants (Bishoi and Prakash, 2009). Further, regulatory AQM stations require certified instrumentation meeting measurement accuracy requirements, and an extensive set of procedures to ensure that data quality remains satisfactory. These requirements, typically required by laws and regulations, ensure that measurements are comparable across all networks with similar requirements, but limit the AQM spatial deployment due to their high investment and operational cost. As a result, the AQM network has limited ability to account for spatial variability of pollution levels in heterogeneous regions such as urban areas, which in return, renders exposure assessment a very difficult task (Rao et al., 2012). Moreover, the air-inlets of AQM stations are typically located on rooftops or way above the ground (European Environment Agency, 1998), thus misrepresenting the true exposure of any individual at head height.

Recent developments in sensory and communication technologies have made the deployment of portable and relatively low-cost micro sensing units (MSUs) possible. These MSUs can operate as a set of individual nodes, or may be interconnected to form a Wireless Distributed Environmental Sensor Network (WDESN) to measure air pollution over large spatial scales. WDESNs gather high-resolution spatial and temporal data from numerous individual nodes allowing for a better interpolation and the generation of dense pollution maps, which are closer to real-life pollution dispersion scenarios (Kanaroglou et al., 2005). The gaseous sensors mounted on these MSUs are low-power and low-cost, and are based on widely understood amperometric sensor methodologies designed for sensing selected gases at the parts-per-million (ppm) level (Bard and Faulkner, 2001; Mead et al., 2013; Stetter and Li, 2008). Electronic circuitry, which applies signal processing, allows for the detection at the part-per-billion level (Mead et al., 2013). Recent miniaturization of Optical Particles Counters (OPCs) (Gao et al., 2016; Ulanowski et al., 2013) and solid state (Carminati et al., 2014, 2015) sensors allows to extend the MSUs capabilities to measure particulate matter (PM) as well.

The small size and low power-consumption of MSUs lay the path for many new applications that require AQ data, such as exposure analyses (Jerret et al., 2005; Lebret, 1990), education (Ballantyne et al., 2010), hot-spot identification and characterization (Ma et al., 2008), supplementary network monitoring (Molchanov et al., 2015; The European Parliament and the Council of the European Union, 2008), and citizen science (Bonney et al., 2009; Shirk et al., 2012; Williams et al., 2014). In particular, the essence of citizen science requires active participation of citizens in the scientific research process (Bonney et al., 2009). Within the context of air-quality research, MSUs may be deployed at citizen's homes, monitoring either ambient or indoor air quality in their local environment. An example is the CITI-SENSE project, which aims at developing sensor-based citizen observatories for improving the quality of life in cities (CITI-SENSE Project, 2015).

Seminal studies that evaluate MSUs in pre-field and field trials show that these units indeed can capture air pollution spatio-temporal variation (Becker et al., 2000; Lee and Lee, 2001; Lerner et al., 2015; Mead et al., 2013; Molchanov et al., 2015; Piedrahita et al., 2014; Williams et al., 2013). However, these studies have shown that the MSUs' main limitation is their low accuracy relative to laboratory equipment (Becker et al., 2000; Lee and Lee, 2001; Mead et al., 2013; Piedrahita et al., 2014; Williams et al., 2013) or an AQM station (Mead et al., 2013; Molchanov et al., 2015; Williams et al., 2013).

Previously-used MSU calibration and evaluation measures, i.e., sensitivity (Becker et al., 2000; Lee and Lee, 2001; Mead et al., 2013; Williams et al., 2013), correlation coefficient, ρ , coefficient of determination, R^2 (Lerner et al., 2015; Mead et al., 2013; Molchanov et al., 2015), and the Root Mean Squared Error, RMSE (Lerner et al., 2015; Molchanov et al., 2015) aim at assessing the MSUs' accuracy and capability to capture trends and values of the pollutants' true ambient levels. While these criteria evaluate some aspects of the sensors' performance in many fields, for some applications different criteria covering additional performance aspects may be more adequate (Williams et al., 2014).

Personal exposure studies have supplied participants with MSUs that measured various air pollutants of exposure during daily routines (e.g., (Rabinovitch et al., 2006; Sarnat et al., 2000)). However, exposure is affected by many factors, and thus the variance of the dose response function is typically high and dominates the attributed relative risks/hazard ratios results, regardless of sensors' accuracy (Jerret et al., 2005; Lebret, 1990). Therefore, one common practice for estimating individual exposure is to use a coarse scale (Bishoi and Prakash, 2009; CITI-SENSE Project, 2015; Kyrkilis et al., 2007), rather than the sensors' actual measurement. Educational and citizen science applications typically aim at fostering informal and qualitative awareness. The measuring range in such applications is typically quantized into a binary scale, indicating the presence or absence of a pollutant. These scales and measures, although quantized, can still be used for relational comparison of air-pollution levels among different locations and times. This

motivates the need for a more widely composed set of criteria to characterize the MSUs' actual (field) capabilities. Having such criteria allows for custom-made assessment of sensor's performance looking at properties that are important according to the task and application in hand.

This work presents a comprehensive Sensor Evaluation Toolkit (SET) for evaluating and comparing the AQ-MSUs' performance and its application on 25 sensors deployed in eight cities in Europe, as part of the CITI-SENSE project (CITI-SENSE Project, 2015). The R implementation of the SET is available on the first author's website.

2. Material and methods

MSU evaluation can be executed either in a laboratory, with critical atmospheric ambient conditions measured and controlled, or in an open uncontrolled environment. The laboratory provides calibration against traceable reference standards. In an open, uncontrolled environment, the MSUs are placed in AQM stations and their measurements are compared against those acquired by AQM (reference) equipment. While the SET requires a reference device (dubbed REF) to evaluate the MSU measurements, it does not make any assertion on the nature of this reference equipment. The evaluation involves a comparison of two concentration time-series: one acquired by the MSU, $\{C_k^{MSU}\}$, and one obtained by the reference device, $\{C_k^{REF}\}$. Both time-series should be of equal length, i.e. consist of K measurements, with the measurement acquired more or less simultaneously.

The SET consists of eight performance measures, including the classic measures of RMSE and various correlations (described in Section 2.1). Four new measures, within the SET, are introduced: the *presence* measure that represents the sensor's availability over time (described in Section 2.2); the *source-analysis*, which depicts how accurately a sensor can identify and locate a source (detailed in Section 2.3); the *match* (detailed in Section 2.4) that evaluates the sensor's accuracy when the measured concentrations are transformed into generalized coarse scales; and the *Lower Frequencies Energy Content* (LFE), which measures the MSUs' ability to capture the temporal variability of the observed pollutant (Section 2.5). All measures are then combined into an Integrated Performance Index (IPI) (Section 2.6).

2.1. Root Mean Squared Error and correlation coefficients

The Root Mean Squared Error (RMSE) and the Pearson correlation measures are often used to evaluate MSUs' performance (Kanaroglou et al., 2005; Lerner et al., 2015; Mead et al., 2013; Molchanov et al.,

2015; Williams et al., 2013). However, these measures apply specific assumptions on the errors and their distributions. RMSE measures the total bias (deviation) between two time series, and is often used to evaluate MSU errors (Mead et al., 2013; Molchanov et al., 2015; Williams et al., 2013). While the RMSE is an excellent general-purpose error metric for numerical deviations, it severely amplifies and disproportionately accounts for large errors. Thus, if two signals have the same values but a small abrupt large deviation the inter-unit RMSE will be large.

Correlation coefficients are often used for evaluating the similarity between two time series, usually in complement to the RMSE (Mead et al., 2013; Molchanov et al., 2015; Williams et al., 2013). Correlation coefficients are robust to abrupt, large deviations and are bounded between $[-1, 1]$, a property which will be exploited in our aggregation process (see Section 2.6). Typically, the correlation of the tested device with a reference is reported with the Pearson correlation coefficient (e.g., (Kanaroglou et al., 2005; Lerner et al., 2015; Mead et al., 2013; Molchanov et al., 2015; Williams et al., 2013)). However, the commonly used Pearson correlation coefficient, ρ , measures how well AQM measurements can be represented by the MSU records using a linear function. This measure is adequate if both the AQM and the MSU are in their linear sensitivity range. Ambient pollutant levels are often below the linear range of the MSUs (Becker et al., 2000; Lee and Lee, 2001; Piedrahita et al., 2014; Williams et al., 2013). Therefore, the SET includes also the Kendall- τ (Daniel, 1990; Kendall, 1948) and the Spearman rank correlation coefficients, S (Myers et al., 2010), which do not assume normality of the underlying variables and perhaps more importantly, are more sensitive to monotonic but non-linear relationships. A real-life example of using the differently defined correlation coefficients is given in Section S1 of Supplementary information. The example presents seven NO MSUs (CitiSense Leo Model, Ateknea Solutions Catalonia, Spain), which are evaluated against a reference AQM for 20 days. While the Pearson and Kendall- τ coefficients are relatively low, and would have rendered the sensor as inadequate, the Spearman coefficient shows that the sensor is suitable for NO measurements, given linearity is not considered. This phenomenon is due to the low NO ambient levels out of the linear response range of the MSUs (Fishbain and Moreno-Centeno, 2016). Thus, the multiple evaluation criteria allow to better characterize MSUs' suitability to different applications.

2.2. Presence

Each sensor's time series may contain missing values. This may result from the sensor malfunctioning or from communication errors.

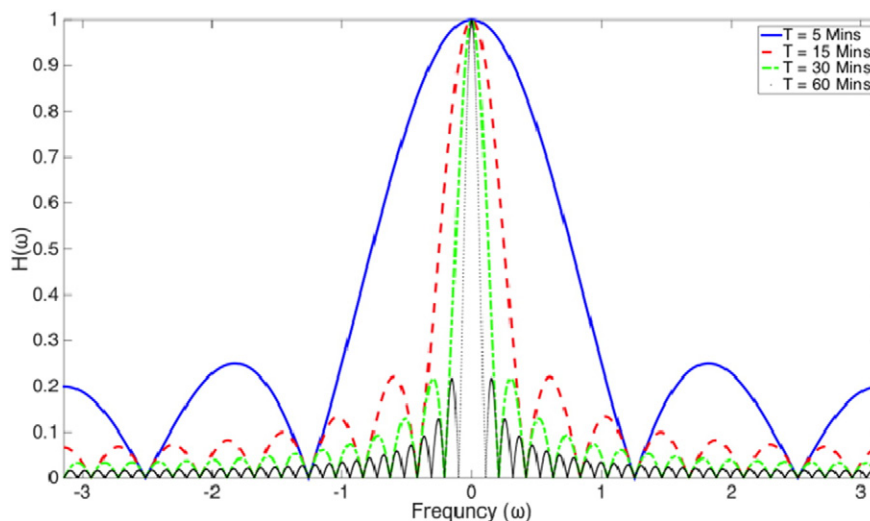


Fig. 1. Fourier Transform of $h(t)$ averaging over 5 min period, i.e. $\Delta t = 5$ min (solid blue); $\Delta t = 15$ min (dashed red); $\Delta t = 30$ min (dot-dash green); and $\Delta t = 60$ min (dotted black).

The *presence* measure accounts for the sensor's or system's availability of a measurement at a given time, and reports the fraction of the acquired measurements of all theoretically possible. The presence of an MSUs is a significant factor in evaluating any outdoor measuring device. For calculating, for example, averages during a given time interval, a minimum data availability is required to ensure representativity. Limited presence always brings about the question of representativity of the measurements for a given environment, and may indicate high maintenance costs. With that, sensor's presence is completely omitted from the RMSE and correlation evaluation criteria.

Standard AQM stations are bounded to standards, connected to the power grid and are placed in dedicated containers, where only the inlets are exposed to outside and weather conditions. Thus, measuring equipment presence is typically a non-issue for AQMs. When it comes to MSUs, presence is often a major hurdle. This is why this measure has a larger significance when evaluating MSUs.

2.3. Source analysis

For many applications such as source apportionment (Carslaw et al., 2006; Westmoreland et al., 2007) or dispersion models, especially Lagrangian models (Carslaw and Ropkins, 2012; Jones et al., 2010), the source location is crucial. Bivariate polar plots, which represent how the concentration of a pollutant varies with the wind direction and speed at the receptor, have proved to be a useful tool for identifying and understanding pollution sources (Carslaw and Ropkins, 2012; Carslaw et al., 2006; Jones et al., 2010; Molchanov et al., 2015; Westmoreland et al., 2007). This representation manifests the directional dependence of different sources, particularly when more than one monitoring site is available, making *source-analysis* ideal for WDES applications.

The source location analysis within the SET aims at evaluating how accurate the MSU is in identifying and locating sources. i.e., it assesses

Table 1
Environmentally sensed indicators - mean values (M) and Integrated Performance Index (IPI) for air pressure (AP); temperature (Temp); relative humidity (RH); nitrogen oxide (NO); nitrogen dioxide (NO₂); ozone (O₃); and carbon monoxide (CO). The IPIs are color coded to represent low to high values in a red-to-green scale.

Unit	Location	AQM Temp [°C]	AP		MSU Temp		RH		NO		NO ₂		O ₃		CO	
			M [mBar]	IPI	M [°C]	IPI	M [%]	IPI	M [ppb]	IPI	Mean [ppb]	IPI	M [ppb]	IPI	M [ppb]	IPI
GAP1	Gal·la Placidia Barcelona Spain	23.62	1007	0.949	24.5	0.887	61.6	0.863	6.2	0.656	13.6	0.464	133.8	0.687	162.9	0.587
GAP2		23.62	1008	0.952	24.5	0.892	62.0	0.864	0.1	0.412	0.8	0.455	178.6	0.669	177.0	0.572
GAP3		23.62	1008	0.950	24.5	0.894	60.8	0.853	1.0	0.557	9.4	0.497	65.4	0.699	137.9	0.584
GAP4		23.62	1008	0.944	24.3	0.897	106.4	0.382	16.2	0.667	9.6	0.503	144.8	0.675	159.0	0.569
GAP5		23.62	1009	0.957	24.5	0.901	68.7	0.543	1.9	0.638	1.8	0.481	153.8	0.674	148.3	0.576
116	St Leonards, Edinburgh, Scotland	7.8	0.513	11.7	0.409	51.2	0.649	58.8	0.524
118		138.0	0.501	8.5	0.394	66.9	0.604	433.3	0.451
120		9.7	0.514	9.9	0.413	42.5	0.627	54.1	0.482
135	Neve Shaannan, Haifa, Israel	12.95	14.7	0.717	57.5	0.860	3.2	0.513	2.7	0.621	71.2	0.663	103.2	0.562
136		12.95	14.4	0.689	57.0	0.842	3.3	0.508	5.0	0.640	44.8	0.697	94.4	0.552
130		12.97	13.6	0.712	57.3	0.829	7.2	0.620	52.3	0.641
134		13.65	14.9	0.705	58.1	0.802	5.9	0.633	41.9	0.633
125	Ljubljana, Slovenia	12.46	979	0.989	13.7	0.935	64.9	0.947	21	0.55	78.4	0.711	166.4	0.769
128		12.46	978	0.940	13.8	0.926	64.8	0.945	3800	0.46	105.8	0.687	175.0	0.681
131		12.46	980	0.934	14.1	0.908	63.6	0.937	6	0.54	96.9	0.719	179.8	0.663
124	Kirkeveien, Oslo, Norway	6.80	1009	0.988	7.9	0.931	84.2	0.889	27.2	0.921	15.5	0.685	101.2	0.710
144		6.80	1007	0.990	7.9	0.945	83.1	0.895	30.5	0.869	16.9	0.637	95.6	0.697
145		6.80	1008	0.989	7.8	0.937	84.5	0.893	23.0	0.860	16.5	0.712	98.8	0.704
146		6.80	1008	0.988	7.9	0.937	84.2	0.896	37.3	0.899	13.7	0.697	102.1	0.682
147		6.80	1008	0.989	7.9	0.945	83.3	0.892	25.9	0.876	14.4	0.565	94.5	0.592
124		7.26	1006	0.976	9.1	0.923	65.9	0.923	16.8	0.859	9.2	0.583
144		7.26	1004	0.993	8.8	0.933	66.9	0.931	16.8	0.871	12.2	0.651
145		7.26	1004	0.992	8.7	0.937	67.0	0.930	11.9	0.795	16.5	0.692
146		7.26	1005	0.978	9.1	0.924	66.2	0.923	9.8	0.732	12.6	0.647
147		7.26	1005	0.991	8.8	0.945	66.4	0.934	16.4	0.856	9.3	0.659
124		17.80	1011	0.983	20.4	0.911	63.0	0.907	15.4	0.842	17.7	0.654
144		17.80	1009	0.991	20.5	0.905	62.8	0.905	15.5	0.843	22.2	0.644
145		17.80	1010	0.989	20.4	0.918	63.7	0.911	5.9	0.760	26.9	0.700
146		17.80	1010	0.986	20.5	0.917	63.1	0.910	22.5	0.803	18.7	0.635
147		17.80	1010	0.988	20.6	0.920	61.9	0.912	12.7	0.828	15.6	0.634
611	Ostrava, Czech Rep.	1.06	992	0.975	4.6	0.901	80.5	0.911	30.5	0.736
612		1.06	991	0.971	4.6	0.896	80.8	0.895	26.3	0.773
221	Belgrade, Serbia	5.78	1008	0.685	5.7	0.885	82.8	0.810	69.7	0.794	27.5	0.591	35.8	0.585	519.8	0.691
222		5.78	1008	0.685	5.7	0.874	81.4	0.815	81.8	0.793	14.3	0.554	60.9	0.537	537.6	0.692
143	Vienna	5.08			15.1	0.473	62.4	0.402	13.2	0.387	5.5	0.348	126.0	0.402
Average IPI				0.953		0.876		0.848		0.711		0.577		0.653		0.617

Table 2

IPI breakdown – mean ambient level (M); match score; Root Mean Squared Error (RMSE); Pearson ρ correlation coefficient; Kendall τ correlation coefficient; Spearman (S) correlation coefficient; source analysis; presence (Pres.); Low Frequencies Energy (LFE) content and the integrated Air Quality Index (IPI).

Sensor	M	Match	RMSE	ρ	τ	S	Source	Pres.	LFE	IPI
118 (NO)	129.9	0.920	0.24	0.063	0.068	0.090	– ^a	0.732	0.976	0.519
130 (T)	13.63	0.462	0.003	0.679	0.538	0.712	– ^a	1	0.997	0.712

^a The Source score could not be computed as no wind data was collected at this location.

the ability of the device to react to changes in observations within a time interval that corresponds to wind direction change, and to be sensitive enough to measure associated changes in concentrations. This is achieved through the calculation of the two-dimensional Pearson correlation between polar plots obtained from the reference device and the MSU, treating both as two-dimensional matrix arrays (Yaroslavsky, 2012). For generating the polar plots, time-matched measurements of the wind and the pollutant must be available. This information is typically obtained either from the AQM station (given it measures these meteorological parameters) or by an externally collocated wind vane. Section S2 of Supplementary material presents an example of a set of two PM_{2.5} MSUs evaluated against an AQM station. While all other performance criteria of the two sensors are relatively similar, the source analysis score of the two sensors does show a difference. This may be attributed to the sensor being placed incorrectly so it has an obscure observation. Thus, a low source analysis score may allow us to find the problem and rectify it.

2.4. Match score

Integrated AQ measures, such as the Air Quality Index (AQI) (Kyrkilis et al., 2007), are often used to convey the general notion of severity of air-quality to the public, ranking observations according to a chosen scheme. Such measures may also be used when the research question does not require precise measurements but rather a more general interpretation, such as general risk estimation (Bishoi and Prakash, 2009; Kyrkilis et al., 2007) and citizen science (Williams et al., 2014). When applying such an AQ grading scheme, neither the RMSE nor the coefficient of determination represent well the sensor's performance, as they penalize small perturbations in the measurements. Thus, if an MSU deviates, due to its inaccuracy, from a reference device and if its deviations are randomly distributed around the reference value, these two measures will report poor performance. The *match score* overcomes this limitation and its calculation is detailed in Algorithm 1.

The match score is the proportion of agreement among strata for increasing amount of sub-partitions between the reference and the MSU measurements. If we would like to compare the different MSUs, the number of maximum sub-partitions, D , should be predetermined and be kept constant throughout the analyses. Its value should be the highest number that still has at least one set of measurements c_t^{MSU} and c_t^{REF} that belong to the same bin. In our analyses, after several preliminary runs, D was set to 10.

Algorithm 1 Match score.

1. Set COUNT = 0
2. Compute the dynamic range for $\{c_t^{MSU}\}$ and for $\{c_t^{REF}\}$, i.e., $[\min\{c_t^{MSU}\}, \max\{c_t^{MSU}\}]$ and $[\min\{c_t^{REF}\}, \max\{c_t^{REF}\}]$ for all $t \in T$.
3. For $d = 1$ to D do:
 - a. Divide MSU's dynamic range into d equal bins and label them 1 through d . Divide REF's dynamic range into d equal bins and label them 1 through d .
 - b. For each pair of measurements $\{c_t^{MSU}, c_t^{REF}\}$, $t \in T$:
If c_t^{MSU} and c_t^{REF} belong to the bins with the same label \rightarrow COUNT = COUNT + 1;
4. Compute: Match Score = $\frac{1}{D \cdot T} \cdot \text{COUNT}$

2.5. Lower Frequencies Energy (LFE)

The signal Lower Frequency Energy, dubbed LFE, is a characteristic of the signal rather than a comparative measure with respect to a reference device. Let us assume that $p(t)$ is a continuous signal that represents the true ambient level of a specific pollutant in a specific location. Both the MSU and the AQM average $p(t)$ over a small sliding temporal-window, $h(t)$, of a size Δt , obtaining $\bar{p}(t)$, and sample it to obtain the aforementioned discrete time series $\{C_k^{MSU}\}$ and $\{C_k^{REF}\}$. Formally, the averaging is described by a convolution integral:

$$\bar{p}(t) = \int_{-\infty}^{\infty} p(\tau)h(t-\tau)d\tau \quad (1)$$

Let ω be the Fourier Transform domain coefficients. Applying the Fourier Transform on $p(t)$ and $h(t)$ (obtaining $P(\omega)$ and $H(\omega)$ respectively) and the convolution theorem (Katznelson, 2004), the Fourier representation of $\bar{p}(t)$, $\bar{P}(\omega)$, is given by:

$$\bar{P}(\omega) = P(\omega) \cdot H(\omega) \quad (2)$$

The Fourier Transform's amplitude of $h(t)$ is presented in Fig. 1 for four different window sizes: averaging over 5, 15, 30 and 60 min. It can be seen that at zero $H(\omega)$ receives a value of one and its value decreases as ω (in absolute value) increases. Considering Eq. (2), the sampling process suppresses higher frequencies, i.e., it applies low-pass filter on the observed signal. Thus, larger window-sizes in the signal domain, i.e. larger Δt , represent narrower filters in the frequency domain.

If the observed pollutant signal changes rapidly, its higher-frequency coefficients will assume higher values. Considering Eq. (2), these values would be diminished in the acquired signal if they are multiplied by a narrow $H(\omega)$, i.e. averaged over a large temporal-window. A real-life example is given in Section S3 in Supplementary material.

The signal's energy is a characteristic used in signal processing and is given by:

$$E = \int_{-\infty}^{\infty} |p(t)|^2 dt \quad (3)$$

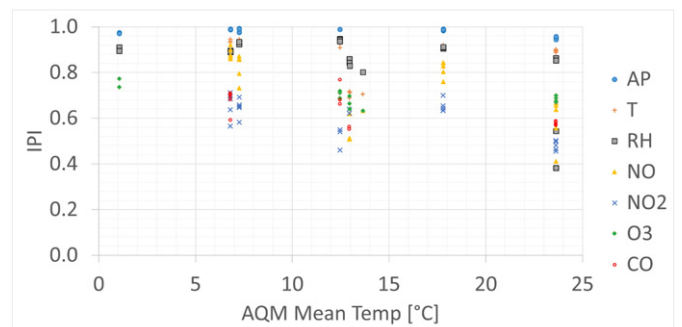


Fig. 2. IPI of the various measured parameters as a function of the ambient temperature.

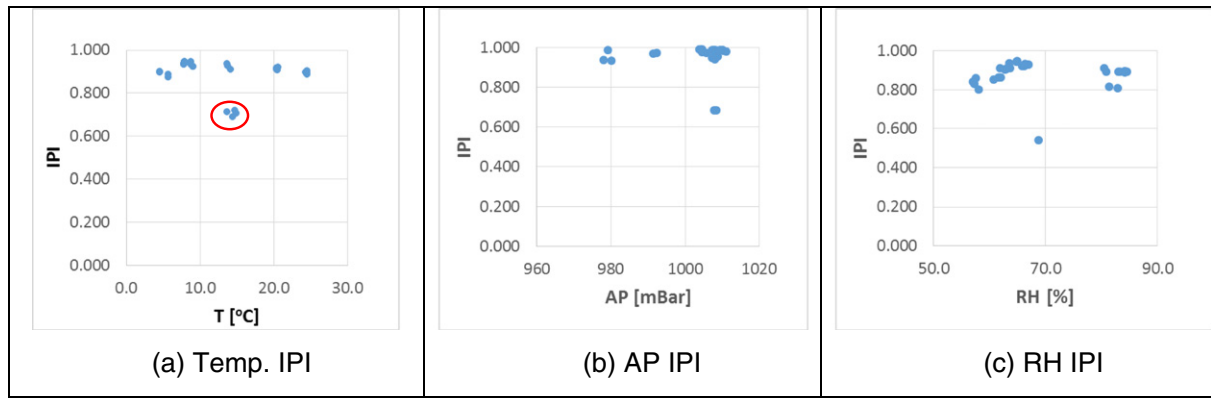


Fig. 3. IPI of a sensor as a function of its specific measured meteorological parameters – temperature IPI (a), air pressure (AP) IPI (b), and relative humidity (RH) IPI (c).

Following the Parseval's theorem (Boas, 2006), the energy of a signal is equal to the energy of its Fourier Transform:

$$E = \int_{-\infty}^{\infty} |P(\omega)|^2 d\omega \quad (4)$$

Hence, the function $|P(\omega)|^2$ represents the energy distribution in the frequency domain. The smaller the energy portion in the higher frequencies, the better the sensor can capture the signal's temporal variability. Thus, the portion of the signal's energy in the lower frequencies, i.e. the *Lower Frequencies Energy* (LFE), can be used for evaluating the sensor's capability to capture the temporal variability of the pollutant. After discrete sampling that accounts for the K samples in the pollution time series Eq. (4) becomes:

$$E = \sum_{\omega=1}^K |P(\omega)|^2, \quad (5)$$

and the LFE measure is computed as:

$$LFE = 1 - \frac{\sum_{\omega=1}^K (\omega \cdot |P(\omega)|^2)}{E \cdot \frac{K(K-1)}{2}} \quad (6)$$

where E is given by Eq. (5).

The maximum value that LFE can obtain is 1, which represents the case where all the information is within the first frequency coefficient, i.e., all frequency coefficients, but the first one, are zero.

MSUs are typically self-contained units with their own power supply and transmission modules. Typically, data acquisition and transmission times are set such that operational energy consumption (for data acquisition and transmission) is minimized. Consequentially, their sampling interval, Δt , may be long, i.e., low sampling rate, which corresponds to narrow low-pass filtering. Therefore, while applicable to AQM and standard laboratory equipment, a measure of spectral distribution is especially important to MSUs working under power consumption constraints.

2.6. Integrated Performance Index (IPI)

The SET consists of eight different performance measures accounting for different aspects of signal acquisition. Different combinations of these measures can be used in order to evaluate the sensor performance, depends on the specific application. In order to integrate the various measures, it is important that they all share the same scale. This is inherent for the SET as all measures span between [0, 1].

Integration of several measures into an overall evaluation measure can be done either by addition or multiplication of all measures together. The former facilitates an aggregation scheme that can account for

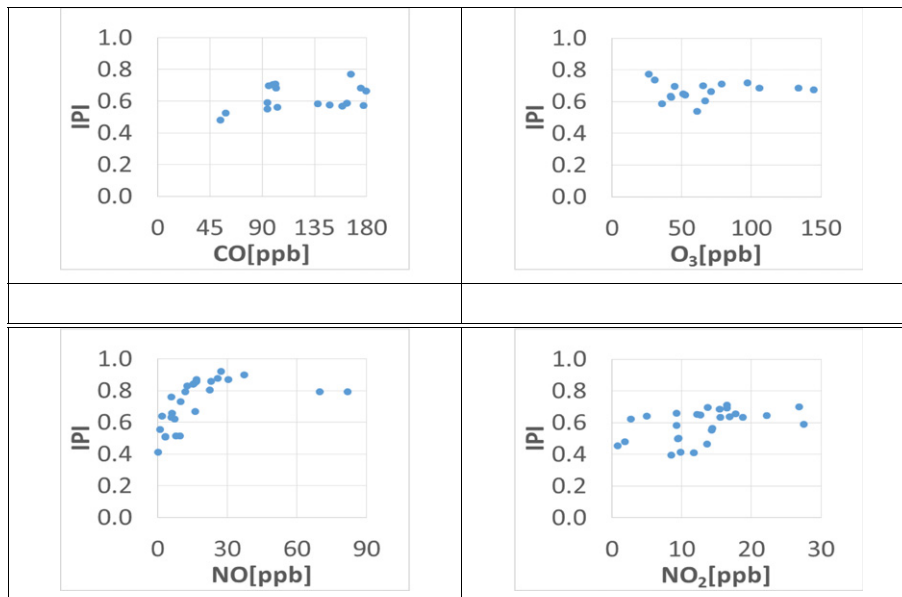


Fig. 4. IPI as a function of pollutants' recorded campaign average levels for each sensor on each node.

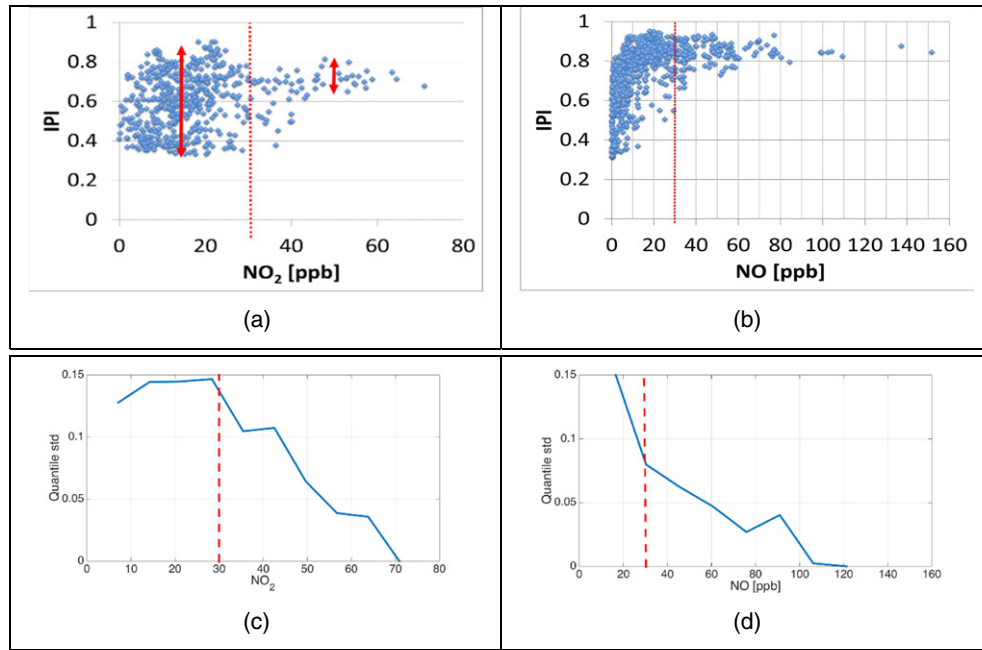


Fig. 5. IPI as a function of NO₂ (a) and NO (b) recorded levels at Kirkeveien, Oslo (daily score). The standard deviation of the IPI computed for each pollution level decile are presented in figures (c) and (d) for NO₂ and NO respectively.

different weights for the different measures by introducing weight coefficients, $\vec{\alpha}$. Given $\vec{\alpha}$, \vec{m} , the measures vector for a given sensor (RMSE, correlations, presence, source analysis, match and LFE), and the time series $\{C_k^{MSU}\}$ and $\{C_k^{REF}\}$ acquired by the sensor and a reference device respectively, the IPI is given by:

$$IPI^{MSU} = \sum_i \alpha_i m_i \left(\{C_k^{MSU}\}, \{C_k^{REF}\} \right) \quad (7)$$

2.7. SET implementation and application

For demonstrating the method and its capabilities, the SET was implemented in R. For evaluation, the MSUs are compared against a reference device. This device can be either AQM or laboratory calibrated equipment. Both the MSU and the reference device must measure the same physical phenomenon (e.g., ambient levels of a specific pollutant, temperature or relative humidity). The same physical phenomenon can be measured when the sensors are collocated (Mead et al., 2013; Molchanov et al., 2015; Williams et al., 2013) or when the observed phenomenon is uniform in all measuring points (Molchanov et al.,

2015; Tsujita et al., 2005). When no AQM nor reference devices are available the same analysis can be done with respect to the average signal of the entire sensory network in a given region (Molchanov et al., 2015). Here we demonstrate the SET for collocated sensors with AQM stations.

For demonstrating the capabilities and richness of the suggested evaluation toolkit, twenty-five MSU pods (Geotech AQMesh, UK, 2015) were placed near ten different AQM stations in eight cities in Europe, as part of the European Union 7th framework program (FP7) CITI-SENSE project (CITI-SENSE Project, 2015). The full deployment, acquiring data for about three months at each location, is detailed in Section S4 of the Supplementary material. Each AQMesh unit was equipped with five environmental sensors: NO, NO₂, O₃, atmospheric pressure (AP), and relative humidity (RH). Some of the AQMesh pods included also OPC PM sensor. Additionally, the AQMesh measured the unit's (internal) temperature (Temp). The specific AQM parameters (location, height above ground level (AGL) and above sea level (ASL)) are detailed in Section S4 of the Supplementary information. The average temperature and the averages of all measured pollutants are provided in Table 1 alongside their SET performance. The latter is color coded to represent low to high SET values in a red-to-green color scale.

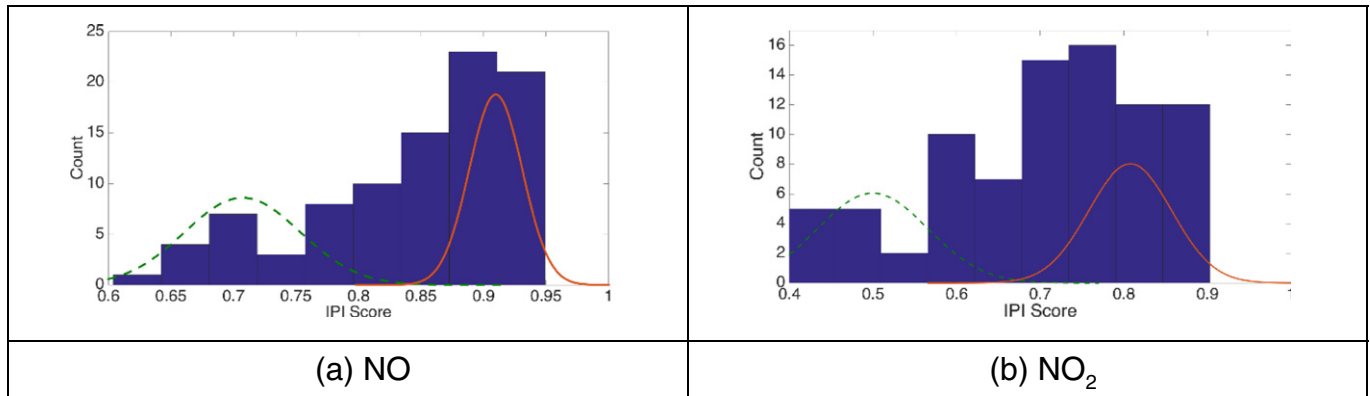


Fig. 6. NO (a) and NO₂ (b) IPI distribution functions measured at Kirkeveien, Oslo (daily score).

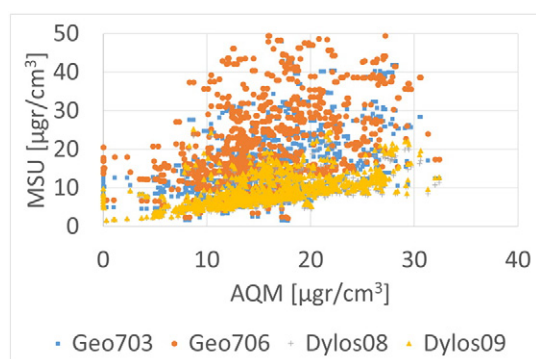


Fig. 7. PM MSU measurements obtained between Dec. 17th and 24th, 2015 plotted against collocated AQM station.

In order to compare the AQM and the MSU measurements, the time resolution of both should be the same. If that is not the case, the finer time resolution time series has been aggregated so it fits the coarser resolution. The MSU time-series were acquired at a 15-min resolution, while the AQM time-series had a 30 (or 60) -min resolution. Hence, MSU measurements were averaged (without overlap) to produce a time-series that corresponds to the AQM temporal resolution.

3. Results and discussion

3.1. Overview

Table 1 depicts the average values of the measured environmental parameters, showing that the MSUs' meteorological measurements are more accurate than those of pollutant concentrations. The AP, (pod internal) Temp and RH sensors have, on average, an Integrated Performance Index (IPI) of 0.975, 0.875 and 0.851, respectively. Among the pollutants, NO sensors had the highest IPI, with an average of 0.705. O₃, CO and NO₂ obtained IPIs of 0.664, 0.609 and 0.578, respectively.

The utilization of the SET for evaluating MSU performance is well demonstrated in Table 1. Sensor 143, which presents lower IPI values for all measured environmental parameters, may have experienced a systematic error. This may result from incorrect placement of the sensor or malfunction of hardware. Sensor GAP 4 presents low IPI for RH. The average RH value that this sensor reported was 106.4%. This clearly suggests that the sensor is faulty or overly-offset for this parameter. Sensor 118 presented low IPI for CO and NO while their average concentrations were much higher than those measured by the AQM and other collocated MSUs. All these measurements were removed from the following analysis.

The richness offered by the IPI is presented in Table 2, through the breakdown of the IPI measure into its components (mean (M), match score, RMSE, Pearson ρ , Kendall τ and Spearman (S) correlation coefficients; source-analysis score, presence (Pres.) and Lower Frequencies Energy (LFE) content) for two sensors – #118 NO and #130 Temp sensors. For both sensors the LFE measure is high, suggesting that the changes in the observed signal are slower than the sampling rate. The #118 NO sensor presents extremely-low correlation values, while its match score is high. Thus, while this specific sensor would grade poorly using the traditional evaluation tools (correlation and RMSE), it would

be more than sufficient for many of the aforementioned applications, such as citizen science and exposure estimations. The Temp sensor of pod #130 also presents interesting behavior. Its Match as well as its correlation coefficients are reasonable, but its RMSE score is very low. This suggests that while the sensor does not represent the true ambient levels, i.e., it has some bias, it does represent the signal's behavior (i.e., good correlations). Indeed, this was the case, as explained in Section 3.3. Therefore we conclude that the different components of the IPI measure do give a better understanding of the sensor performance and its suitability for different applications.

3.2. Temperature impact on the measurements

Ambient temperature has been pointed-out as a major factor affecting sensor performance (Lerner et al., 2015; Mead et al., 2013; Molchanov et al., 2015; Williams et al., 2013). Here we examine this using the IPI. Fig. 2 shows the average IPI of all 25 MSUs for all seven measured parameters, as a function of the average temperature that was measured by the AQM station throughout the campaign. The temperature effect is evaluated over 175 measurements. Each of these 175 measurements consists of more than three months' worth of data. Thus, the temperature evaluation is based on a large dataset. No apparent trend is observed, suggesting that the MSUs manage to compensate for any temperature impact on the measurements. Previously reported temperature effects on AQ measurements may be attributed to higher pollution levels in winter time (due to higher pollution source strength and pollution accumulation during periods with temperature inversions (Seinfeld and Pandis, 2016; Yoshikado and Tsuchida, 1996)). This is because while temperature was not found to affect sensors' performance, the measured ambient levels, as is shown later, do have an effect, where the sensors performs better in higher pollution levels. Next, we analyze the IPI specifically for each measured parameter.

3.3. Meteorological sensors

Fig. 3 presents the IPI for the Temp, AP and RH sensors for all MSUs, as a function of their average values. The first notion that arises from this presentation is that, in general, the sensors' IPI is indifferent to changes in the observed meteorological parameter. It is worthwhile mentioning that the batch of temperature sensors with lower IPI values (marked in circle in Fig. 3a) were all obtained in the same station in Haifa, Israel. Further queries revealed that temperature records in this specific AQM were measured inside the monitoring station rather than outside, where the MSUs were located. This example demonstrates once again the use of the SET to point out sensing errors.

3.4. Gaseous pollutants sensors

Fig. 4 depicts pollutant specific sensor's IPI as a function of the average reading. Thus, the IPI of each pollutant's sensor, computed over the entire campaign, is plotted against the same pollutant's campaign average reading. It is evident from Fig. 4 that the ambient level of the observed pollutant has a direct impact on the sensing quality. The lower the ambient pollutant level, the lower the IPI and the higher its variance for similar pollutant's ambient levels (i.e., the sensors presents lower reliability for lower pollutants ambient levels). Similar behavior was observed by Lerner et al. (2015) and Molchanov et al. (2015). Hence, the IPI suggests that the MSU sensors are more suitable for locations where the pollutant is known to be high. Means to extract the threshold are discussed next. As different pollutants have different ambient levels, it is important to note that the x-axes of all following figures present different scales.

The aforementioned IPI behavior as a function of the pollutant's ambient level is better observed when the IPI is computed based on a daily time series rather than using the entire campaign's time series. For example, Fig. 5, depicts the daily IPI for NO₂ (a) and NO (b) from

Table 3

IPI breakdown of PM sensors. The scores are color coded to represent low to high values in a red-to-green scale.

	Mean	Match	RMSE	Pearson	Kendall	Spearman	Presence	eBalance	IPI
Geo703	23.766	0.101	0.038	0.147	0.309	0.453	1.000	0.982	0.565
Geo706	26.926	0.119	0.023	0.259	0.284	0.421	1.000	0.993	0.579
Dylos08	139.894	0.311	0.134	0.560	0.468	0.639	1.000	0.997	0.693
Dylos09	152.258	0.312	0.147	0.570	0.474	0.647	1.000	0.997	0.695

measurements obtained in Kirkeveien, Oslo, by sensors #124, #144, #145, #146 and #147 (see Section S4). One should determine the minimum ambient levels a sensor can measure where the IPI measure is high and the standard deviation is low (how high and how low is application dependent). Figures (c) and (d) depict the standard deviation of the IPI, computed for the associated IPIs of each decile of the pollution levels. It is evident that the standard deviation decreases as the IPI increases. Using the notions above, a sensible threshold for the sensors described for measuring NO₂ and NO can be ambient levels that are higher than 30 ppb.

Fig. 6 demonstrates the utilization of the IPI for comparison between sensors and between different working conditions; The figure depicts the histograms of the NO and NO₂ levels at Kirkeveien, Oslo, which are presented in Fig. 5 (as time series). The notion above, of the effect of ambient levels on the sensors' performance, is evident in Fig. 6, where a bimodal distribution of the IPI is well observed. The two models correspond to IPI scores above and below 30 ppb. Having the bimodal distributions' parameters inferred, one can study their relations. Formally, this can be done by the Kolmogorov-Smirnov test for discrete variables (Arnold and Emerson, 2001; Smirnov, 1948) comparing the best fitting distribution with the empirical distribution and test for significance.

3.5. Particulate matter sensors

The SET criteria was applied to four different PM sensors, all collocated at the Igud AQM station (Haifa, Israel – see Table 1). The four sensors, two DC1700 Dylös (US) and two optical counters integrated on the GeoTech MSUs, were placed next to the AQM's inlet between December 17th and 24th, 2015. The data was recorded in 5 minute intervals. The four sensors measurements are displayed against AQM PM measurements, where all measurements are in [$\mu\text{g}/\text{m}^3$] (Fig. 7).

Table 3 shows the IPI breakdown for the PM sensors. The two types of sensors present different characteristics, while the GeoTech sensors present better RMSE, the Dylös ones have better match, correlations and eBalance. Thus, the SET is also capable to evaluate PM sensors and define better the suitability of a sensor to a specific application.

4. Conclusions

This paper presents a Sensor Evaluation Toolbox (SET) for evaluating AQ MSUs by a range of criteria. The rich evaluation provided by the suggested scheme allows for better assessment of sensors' performance in varied applications and environments. The SET consists of eight different assessment criteria: Root Mean Squared Error (RMSE), Pearson, Kendall and Spearman correlations, and four new performance measures for evaluating sensors' capability to: locate pollution sources; represent the pollution level on a coarse scale; capture the high temporal variability of the observed pollutant and their reliability.

Application of the SET on measurements acquired by gaseous and PM MSUs deployed in eight cities across Europe showed that each of the eight measures provides an important and unique information on the sensor's performance assessing a rich spectrum of MSU capabilities. The result also demonstrates how the scheme can pinpoint systematic as well as sensor's specific faults. Further, we demonstrated that the Integrated Performance Index (IPI) can support a methodology for determining the sensors' performance, hence facilitating a true cross platform evaluation. The SET was implemented in R (Zumel and Mount, 2014) and is available on the first author's website.

Acknowledgements

We would like to acknowledge the AQM station managers for providing ambient air quality data, including the Haifa District Municipal Association for Environmental Protection (Israel); Xarxa de Vigilància i

Previsió de la Contaminació Atmosfèrica de Catalunya (XVPCA), Direcció General de la Qualitat Ambiental, Departament de Territori i Sostenibilitat, Generalitat de Catalunya (Spain); the Slovenian Environment Agency (Slovenia); the Czech Hydrometeorological Institute (Czech Republic); Bureau Veritas, UK Ltd. (Edinburgh); the Serbian Environmental Protection Agency – SEPA (Serbia).

CITI-SENSE, initiated in October 2012, is a four year Collaborative Project partly funded by the EU FP7-ENV-2012 under grant agreement 308524.

Appendix A. Supplementary data

Supplementary data to this article can be found online at <http://dx.doi.org/10.1016/j.scitotenv.2016.09.061>.

References

- AQMesh, UK, 2015. AQMesh website July [Online]. Available: <http://www.aqmesh.com> (Accessed July 2015).
- Arnold, T.B., Emerson, J.W., 2001. Nonparametric goodness-of-fit tests for discrete null distributions. *The R Journal* 3 (2), 34–39.
- Ballantyne, R., Fien, J., Packer, J., 2010. Program effectiveness in facilitating intergenerational influence in environmental education: lessons from the field. *J. Environ. Educ.* 32 (4), 8–15.
- Bard, A., Faulkner, L., 2001. *Electrochemical Method: Fundamentals and Application*. 2 ed. John Wiley & Sons, New-York, NY, USA.
- Becker, T., Muhlberger, S., Braunnmuhl, C., Muller, G., Ziemann, T., Hechtenberg, K., 2000. Air pollution monitoring using tin-oxide-based micro-reactor system. *Sensors Actuators B* 69, 108–119.
- Bishoi, B., Prakash, A., 2009. A comparative study of air quality index based on factor analysis and US-EPA methods for an urban environment. *Aerosol Air Qual. Res.* 9 (1), 1–17.
- Boas, M., 2006. *Mathematical Methods in the Physical Sciences*. John Wiley & Sons, Hoboken, NJ, USA.
- Bonney, R., Ballard, H., Jordan, R., McCallie, E., Phillips, T., Shirk, J., Wilderman, C.C., 2009. Public Participation in Scientific Research: Defining the Field and Assessing Its Potential for Informal Science Education.
- Carminati, M., Pedalà, L., Bianchi, E., Nasonb, F., Dubini, G., Cortelezzi, L., 2014. Capacitive detection of micrometric airborne particulate matter for solid-state personal air quality monitors. *Sensors Actuators A Phys.* 219, 80–87.
- Carminati, M., Ferrari, G., Sampietro, M., 2015. Emerging miniaturized technologies for airborne particulate matter pervasive monitoring. *Measurement*.
- Carlsaw, D., Ropkins, K., 2012. Openair d An R package for air quality data analysis. *Environ. Model. Softw.* 27–28, 52–61.
- Carlsaw, D., Beevers, S., Ropkins, K., Bell, M., 2006. Detecting and quantifying aircraft and other on-airport contributions to ambient nitrogen oxides in the vicinity of a large international airport. *Atmos. Environ.* 40 (28), 5424–5434.
- CITI-SENSE Project, 2015. Home page. [Online]. Available: <http://www.citi-sense.eu> (Accessed 01 04 2015).
- Crouse, D., Goldberg, M., Ross, N., 2009. A prediction-based approach to modelling temporal and spatial variability of traffic-related air pollution in Montreal, Canada. *Atmos. Environ.* 43 (32), 5075–5084.
- Daniel, W., 1990. Kendall's tau. *Applied Nonparametric Statistics*. PWS-Kent, Boston, pp. 365–377.
- European Environment Agency, 1998. *Assessment and Management of Urban Air Quality in Europe*. Office for Official Publications of the European Communities, Denmark.
- Fishbain, B., Moreno-Centeno, E., 2016. "Self calibrated wireless distributed environmental sensory networks". *Sci. Report.* 6, 24382–24391.
- Gao, R.S., Telg, H., McLaughlin, R.J., Ciciora, S.J., Watts, L.A., Richardson, M.S., Schwarz, J.P., Perring, A.E., Thornberry, T.D., Rollins, A.W., Markovic, M.Z., Bates, T.S., Johnson, J.E., Fahey, D.W., 2016. A light-weight, high-sensitivity particle spectrometer for PM_{2.5} aerosol measurements. *Aerosol Sci. Technol.* 50 (1), 88–99.
- International Agency for Research on Cancer (IARC), 2013. *Ambient air pollution*. IARC Meeting Monographs (Lyon, France).
- Jerret, M., Arain, A., Kanaroglou, P., Beckerman, B., Potoglou, D., Sahuvaroglu, T., Morrison, J., Giovis, C., 2005. A review and evaluation of intraurban air pollution exposure models. *J. Expo. Anal. Environ. Epidemiol.* 15, 185–204.
- Jones, A., Harrison, R., Baker, J., 2010. The wind speed dependence of the concentrations of airborne particulate matter and Nox. *Atmos. Environ.* 44 (13), 1682–1690.
- Kanaroglou, P., Jerrett, M., Morrison, J., Bernardo Beckerman, M., Arain, A., Gilbert, N., Brook, J., 2005. Establishing an air pollution monitoring network for intra-urban population exposure assessment: a location-allocation approach. *Atmos. Environ.* 39 (13), 2399–2409.
- Katznelson, Y., 2004. Ch. 1 - Fourier series on T. *An Introduction to Harmonic Analysis*. Cambridge University Press, Cambridge, UK, pp. 1–54.
- Kendall, M., 1948. *Rank Correlation Methods*. Charles Griffin & Company Limited, London.
- Kyrkili, G., Chaloulakou, A., Kassomenos, P., 2007. Development of an aggregate Air Quality Index for an urban Mediterranean agglomeration: relation to potential health effects. *Environ. Int.* 33 (5), 670–676.
- Lebre, E., 1990. Error in exposure measures. *Toxicol. Ind. Health* 6, 147–156.
- Lee, D., Lee, D., 2001. Environmental gas sensors. *IEEE Sensors J.* 1 (3), 214–224.

- Lerner, U., Yacobi, T., Levy, I., Moltchanov, S., Cole-Hunter, T., Fishbain, B., 2015. The effect of ego-motion on environmental monitoring. *Sci. Total Environ.* 533, 8–16.
- Ma, Y., Richards, M., Ghanem, M., Guo, Y., Hassard, J., 2008. Air pollution monitoring and mining based on sensor grid in London. *Sensors* 8 (6), 3601–3623.
- Mead, M., Popoola, O., Stewart, G., Landshoff, P., Calleja, M., Hayes, M., Baldovi, J., McLeod, M., Hodgson, T., Dicks, J., Lewis, A., Cohen, J., Baron, R., Saffell, J., Jones, R., 2013. The use of electrochemical sensors for monitoring urban air quality in low-cost, high-density networks. *Atmos. Environ.* 70, 186–203.
- Molchanov, S., Levy, I., Etzion, Y., Lerner, U., Broday, D., Fishbain, B., 2015. On distributed air quality measurements with micro sensors. *Sci. Total Environ.* 502, 537–547.
- Myers, J., Well, A., Jr, R.L., 2010. Inference, assumptions, and power in multiple regression. *Research Design and Statistical Analysis*. Lawrence Erlbaum, New-York, NY, USA, pp. 551–572.
- Piedrahita, R., Xiang, Y., Masson, N., Ortega, J., Collier, A., Jiang, Y., Li, K., Dick, R., Lv, Q., Hannigan, M., Shang, L., 2014. The next generation of low-cost personal air quality sensors for quantitative exposure monitoring 7, 33. *Atmos. Meas. Tech.* 7, 3325–3336.
- Pope, C., Burnett, R., Thun, M., Calle, E., Krewski, D., Ito, K., Thurston, G., 2002. Lung cancer, cardiopulmonary mortality, and long-term exposure to fine particulate air pollution. *JAMA* 287 (9), 1132–1141.
- Rabinovitch, N., Strand, M., Gelfand, E., 2006. Particulate levels are associated with early asthma worsening in children with persistent disease. *Am. J. Respir. Crit. Care Med.* 173 (10), 1098–1105.
- Rao, S., Chirkov, V., Dentener, F., Dingenen, R., Pachauri, S., Purohit, P., Amann, M., Heyes, C., Kinney, P., Kolp, P.K.Z., Riahi, K., Schoepp, W., 2012. Environmental modeling and methods for estimation of the global health impacts of air pollution. *Environ. Model. Assess.* 17 (6), 613–622.
- Sarnat, J., Koutrakis, P., Suh, H., 2000. Assessing the relationship between personal particulate and gaseous exposures of senior citizens living in Baltimore, MD. *J. Air Waste Manage. Assoc.* 50 (7), 1184–1198.
- Seinfeld, J.H., Pandis, S.N., 2016. *Atmospheric Chemistry and Physics: From Air Pollution to Climate Change*. John Wiley & Sons.
- Shirk, J., Ballard, H., Wilderman, C., Phillips, T., Wiggins, A., Jordan, R., McCallie, E., Lewenstein, B., Krasny, M., Bonney, R., 2012. Public participation in scientific research: a framework for deliberate design. *Ecol. Soc.* 17 (2).
- Smirnov, N., 1948. Table for estimating the goodness of fit of empirical distributions. *Ann. Math. Stat.* 19, 279–281.
- Stetter, J.R., Li, J., 2008. Amperometric gas sensors a review. *Chem. Rev.* 108 (2), 352–366.
- The European Parliament and the Council of the European Union, "Directive 2008/50/EC on ambient air quality and cleaner air for Europe," Off. J. Eur. Union, pp. L152/1–L152/44, (21 May) 2008.
- Tsujita, W., Yoshino, A., Ishida, H., Moriizumi, T., 2005. Gas sensor network for air-pollution monitoring. *Sensors Actuators B* 110, 304–311.
- Ulanowski, J., Kaye, P., Hirst, E., Wieser, A., Stanley, W., 2013. Miniature, low-cost optical particle counters. *Int. Conf. Optical Characterization of Atmospheric Aerosols, Smolenice, Slovakia*.
- Westmoreland, E., Carslaw, N., Carslaw, D., Gillah, A., Bates, E., 2007. Analysis of air quality within a street canyon using statistical and dispersion modelling techniques. *Atmos. Environ.* 41 (39), 9195–9205.
- Williams, D., Henshaw, G., Bart, M., Laing, G., Wagner, J., Naisbitt, S., Salmond, J., 2013. Validation of low-cost ozone measurement instruments suitable for use in an air-quality monitoring network. *Meas. Sci. Technol.* 24 (6), 5803–5814.
- Williams, R., Kilaru, V., Snyder, E., Kaufman, A., Dye, T., Rutter, A., Russell, A., Hafner, H., 2014. *Air Sensor Guidebook*. National Exposure Research Laboratory, Office of Research and Development, U.S. Environmental Protection Agency, Research Triangle Park, NC, USA.
- Yaroslavsky, L., 2012. *Theoretical Foundations of Digital Imaging Using MATLAB*. CRC Press.
- Yoshikado, H., Tsuchida, M., 1996. High levels of winter air pollution under the influence of the urban heat island along the shore of Tokyo Bay. *J. Appl. Meteorol.* 35 (10), 1804–1813.
- Zumel, N., Mount, J., 2014. *Practical Data Science With R*. Manning, Shelter Island, NY, USA.